



GRL Platform Solutions

USB4® Return Loss Test Method of Implementation (MOI) & User Guide Using Anritsu MS46524B Vector Network Analyzer and GRL-USB4RL-AN Automation Software

Published on 04 May 2026

DISCLAIMER

This document is provided “as is” with no warranties whatsoever, including any warranty of merchantability, no infringement, fitness for any particular purpose, or any warranty otherwise arising out of any proposal, specification, or sample. The GRL Platform Solutions disclaims all liability for infringement of proprietary rights, relating to use of information in this specification. No license, express or implied, by estoppel or otherwise, to any intellectual property rights is granted herein.

All product names are trademarks, registered trademarks, or service marks of their respective owners.



Copyright © 2026 GRL Platform Solutions. All rights reserved.

TABLE OF CONTENTS

1	INTRODUCTION	6
2	RESOURCE REQUIREMENTS	7
2.1	EQUIPMENT REQUIREMENTS	7
2.2	SOFTWARE REQUIREMENTS	8
3	INSTALLATION AND SETUP OF GRL-USB4RL-AN SOFTWARE	9
3.1	DOWNLOAD GRL-USB4RL-AN SOFTWARE.....	9
3.1.1	Connect Anritsu Vector Network Analyzer with PC.....	11
3.1.2	Download and Install USB4 Electrical Test Tools (ETT)	12
3.1.3	Launch and Set Up Software.....	13
4	TIME AND FREQUENCY DOMAIN CALIBRATION SETUPS	15
5	CALIBRATING WITH GRL-USB4RL-AN SOFTWARE	17
5.1	SELECT CALIBRATION	17
5.2	CONFIGURE CALIBRATION PARAMETERS.....	18
5.3	RUN CALIBRATION	19
6	CONFIGURE PROPER SETUP IN CONFIGURATIONS MENU	20
6.1	HOST DUT SETUP.....	20
6.2	DEVICE DUT SETUP FOR UFP.....	21
6.3	DEVICE DUT SETUP FOR DFP.....	21
7	PERFORM TRACE GATING	22
8	DUT COMPLIANCE TESTING WITH GRL-USB4RL-AN SOFTWARE	23
8.1	SELECT TESTS	23
8.2	CONFIGURE TEST PARAMETERS.....	24
8.3	PERFORMING IMPEDANCE AND RETURN LOSS MEASUREMENT.....	25
9	TEST RESULTS AND REPORTS WITH GRL-USB4RL-AN SOFTWARE	27
9.1	GENERATE TEST REPORT.....	27
9.1.1	DUT Information	27
9.1.2	Summary Table.....	28
9.1.3	Test Result Details.....	28
9.2	DELETE REPORTS.....	29
10	TROUBLESHOOTING GRL-USB4RL-AN ERRORS	30

List of Figures

Figure 1. Launching GRL Platform Solutions Software Framework.....	9
Figure 2. Start GRL-USB4RL-AN Application.....	10
Figure 3. See License Details.....	10
Figure 4. Check License for Installed Application	10
Figure 5. Connecting Anritsu VNA with Control PC	11
Figure 6. Setting VNA and PC Network	11
Figure 7. GRL-USB4RL-AN IP Addressing on VNA.....	13
Figure 8. Session Info Page	13
Figure 9. Select Test Port.....	14
Figure 10. Select Data Rate	14
Figure 11. Calibration Setup for Time Domain Calibration.....	15
Figure 12. Calibration Setup for Frequency Domain Calibration	15
Figure 13. Software Calibration Guide Example	16
Figure 14. Select Calibration Types.....	17
Figure 15. Calibration Configuration Page.....	18
Figure 16. Run Tests Page.....	19
Figure 17. Test Setup for Host DUT	20
Figure 18. Configure Host DUT Example in GRL-USB4RL-AN Software	21
Figure 19. Configure Device DUT (UFP) Example in GRL-USB4RL-AN Software	21
Figure 20. Select Trace Gating	22
Figure 21. Run Trace Gating.....	22
Figure 22. Select Rx Measurement Tests	23
Figure 23. Select Tx Measurement Tests	23
Figure 24. Test Configuration Page.....	24
Figure 25. Run Tests Page	25
Figure 26. View Test Results Example.....	26
Figure 27. Generate Report Page	27
Figure 28. DUT Information.....	27
Figure 29. Summary Table	28
Figure 30. Test Result Details Example.....	28
Figure 31. Delete Individual Calibration/Test Results Example.....	29
Figure 32. Delete All Results.....	29

List of Tables

Table 1. Equipment Requirements – Systems.....	7
Table 2. Equipment Requirements – Accessories.....	7
Table 3. Software Requirements	8
Table 4. Calibration Parameters.....	18
Table 5. Run Options.....	19
Table 6. Test Parameters	24

1 Introduction

This MOI & User Guide documentation describes how to perform automated Calibration and Testing of the USB4® Return Loss using Anritsu (MS46524B) Vector Network Analyzer and GRL-USB4RL-AN Automation Software.

The GRL-USB4RL-AN automation software includes calibrating for time and frequency domain and measuring impedance and return loss for USB4 devices under test. When combined with a satisfactory level of interoperability testing, these tests provide a reasonable level of confidence that the device under test will function properly in many USB4 environments.

This MOI & User Guide documentation mainly covers the following for USB4 Return Loss calibration and testing.

1. Equipment required for calibration and testing.
2. GRL-USB4RL-AN Automation Software setup for calibration and testing.
3. Specification Standard automated calibration and test procedures.

2 Resource Requirements

2.1 Equipment Requirements

TABLE 1. EQUIPMENT REQUIREMENTS – SYSTEMS

System	Qty.	Description	Key Specification
Vector Network Analyzer (VNA)	1	Anritsu MS46524B ShockLine™ 4-Port Performance Vector Network Analyzer - MS46524B-020 – Frequency Domain option (50 kHz to 20 GHz) - MS46524B-002 – Time Domain option (with time gating) Firmware Version: V2018.2.1 or above	40GHz 140dB max

TABLE 2. EQUIPMENT REQUIREMENTS – ACCESSORIES

Accessory	Qty.	Description	Key Specification
Computer	1	External PC for running GRL-USB4RL-AN Software	Windows 7+ OS
Calibration Kit	1	Anritsu TOSLKF50A-20 Coaxial Calibration Kit	Type K(f), DC to 20GHz, 50 ohms
USB4 Microcontroller	1	Wilder-Tech USB4 Gen3 μ Controller (USB4-TPA-UC-K, Kit Part No. 640-0961-000)	Optional for some test configurations, see Section 3.1.2
USB4 Test Fixture	1	Wilder-Tech USB4 CIO Plug board (USB4-TPA-UC-K, Kit, Part No. 600-1191-100)	
SMA-SMP Adapter or SMA-SMP Cables	4	Rosenberger 02K118-K00S3 Straight RPC-2.92 Jack-Mini-SMP Jack Adapter - Or - Wilder-Tech Part No. 415-0080-004 – 9” High Performance Phase Aligned Flexible Coaxial Cables w/ Female 2.92mm to Female SMP	DC to 40 GHz, 50 ohms
Matched Cable Pairs	2 pairs	Rosenberger UFC142A 2.92m (x2), 1m SMA cable	Phase matched $\pm 2^\circ$ at 40GHz Insertion loss 1dB max in 10GHz

Note that gentle handling of the fixture coaxial cable connections is required to avoid damage. For instance, when connecting to the fixture, the coaxial cables should not be twisted, bended, or have tension applied where possible. The fixture should also be connected to the DUT prior to making any SMP connections. Refer to the user documentation by Wilder Technologies for the full list of precaution steps to observe when using the cables.

2.2 Software Requirements

TABLE 3. SOFTWARE REQUIREMENTS

Software	Source
GRL-USB4RL-AN	GRL Platform Solutions USB4 Return Loss Calibration and Test Automation Software – www.grlps.com (Support > Download Center)
VISA (Virtual Instrument Software Architecture) API Software	VISA Software is required to be installed on the host PC running GRL-USB4RL-AN software. GRL Platform Solutions' software framework has been tested to work with all three versions of VISA available on the Market: 1. NI-VISA: http://www.ni.com/download/ni-visa-17.0/6646/en/ 2. Keysight IO Libraries: www.keysight.com (Search on IO Libraries) 3. Tektronix TekVisa: www.tek.com (Downloads > Software > TekVisa)
USB4 Electrical Test Tool (ETT)	Downloadable from USB-IF's website. See Section 3.1.2 for more details.

3 Installation and Setup of GRL-USB4RL-AN Software

This section provides procedures for installing, configuring, and verifying the operation of the GRL-USB4RL-AN software and USB4 electrical test toolset. It also helps you familiarize with the basic operation of the GRL-USB4RL-AN software.

The software installer automatically creates shortcuts in the Desktop and Start Menu.

To open the application, follow the procedure in the following section.

3.1 Download GRL-USB4RL-AN Software

Install, launch and set up the GRL-USB4RL-AN software on a PC (where the GRL-USB4RL-AN is referred to as 'Control PC' in this MOI & User Guide).

1. Install VISA (Virtual Instrument Software Architecture) on to the PC where GRL-USB4RL-AN is to be used (see Section 2.2).
2. Download the software ZIP file package from the GRL Platform Solutions support site.
3. The ZIP file contains:
 - **AnritsuUSB4ReturnLoss00xxxxxxxSetup.exe** – Run this on the PC to install the application.
 - **AnritsuUSB4ReturnLossSetupFileInstallation00xxxxxxxSetup.exe** – Run this on the VNA to install the proper setup files.
4. Launch and set up the GRL-USB4RL-AN software as follows:
 - a) Open the **GRL** folder from the Windows Start Menu. Click on **GRL – Automated Test Solutions** within the GRL folder to launch the GRL Platform Solutions software framework.

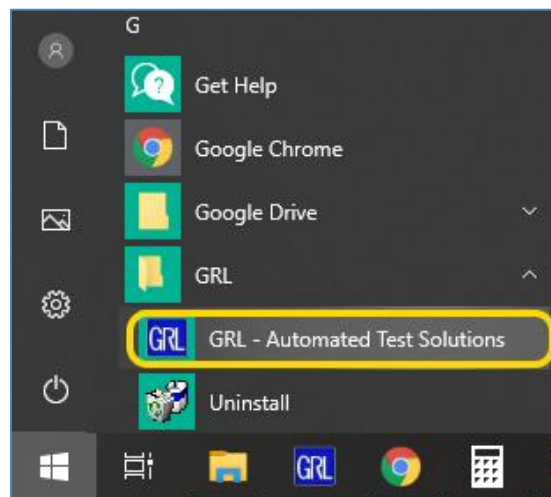


FIGURE 1. LAUNCHING GRL PLATFORM SOLUTIONS SOFTWARE FRAMEWORK

- b) From the **Application → Framework Test Solution** drop-down menu, select **Anritsu USB4 Return Loss Test Application**. If the selection is grayed out, it means your license has expired.

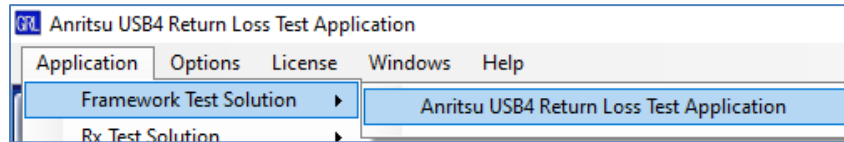


FIGURE 2. START GRL-USB4RL-AN APPLICATION

- i) To enable license, go to **License** → **License Info**.




FIGURE 3. SEE LICENSE DETAILS

- ii) Check the license status for the installed application.

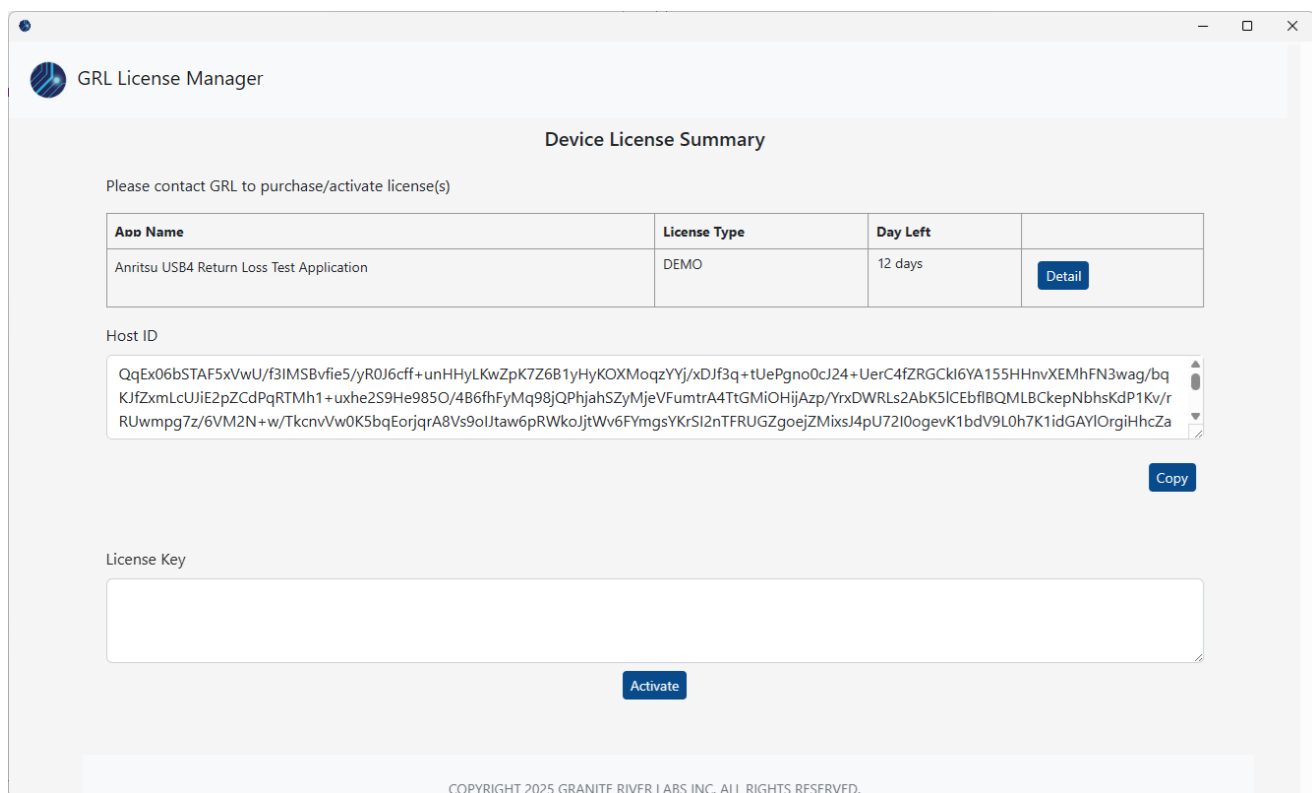


FIGURE 4. CHECK LICENSE FOR INSTALLED APPLICATION

- iii) Activate a License:

- If you have an Activation Key, enter it in the **License Key** field provided and select **Activate**. The installed application is ready for use upon successful activation.
- If you do not have an Activation Key, close the above window to use a demo version of the application over a free 12-day trial period.

Note: Once the 12-day trial period ends, you will need to request an Activation Key to continue using the application on the same computer by contacting support@grlps.com.

3.1.1 Connect Anritsu Vector Network Analyzer with PC

1. Connect the Anritsu VNA with the control PC using an Ethernet cable.



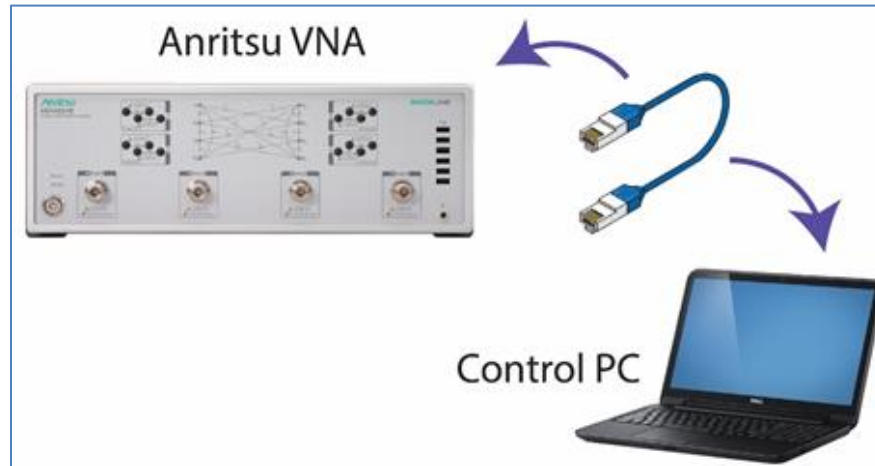


FIGURE 5. CONNECTING ANRITSU VNA WITH CONTROL PC

2. Set both VNA and PC to the same network.

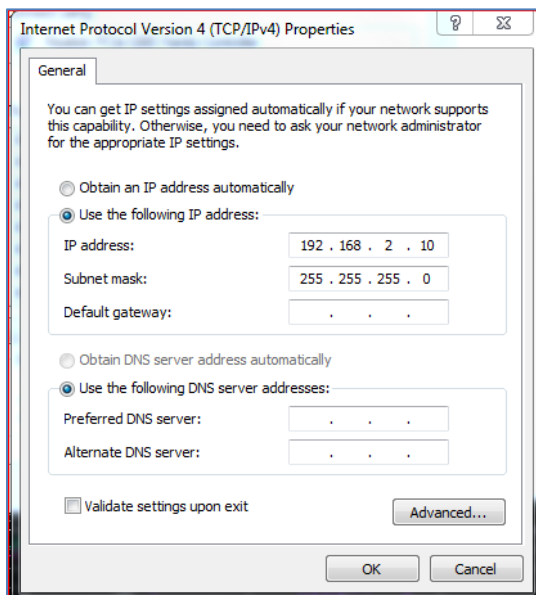

VNA

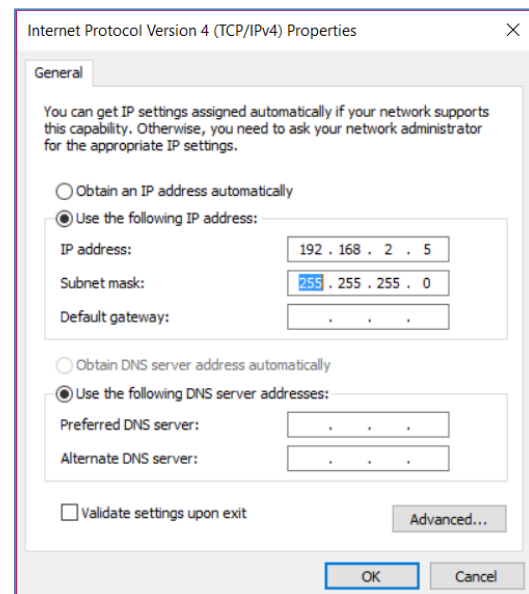

Control PC

FIGURE 6. SETTING VNA AND PC NETWORK

3.1.2 Download and Install USB4 Electrical Test Tools (ETT)


For USB4 Return Loss measurements, the Host/Device's CIO PHY must be in an active state during testing. Its transmitters shall be transmitting PRBS-31 into the VNA measurement channel during testing and its receivers shall have their terminations enabled during testing. Thus, a PHY microcontroller must be used to put the DUT into the right state for return loss testing.

Download ETT:

Visit the USB-IF official website and download "USB4 Electrical Test Tool" (ETT) at <https://www.usb.org/usb4tools>.

Install ETT:

Before running ETT, configure the Control PC's environment using the instructions in **USB4ETT_Documentation.pdf** from the ETT package downloaded from USB-IF.

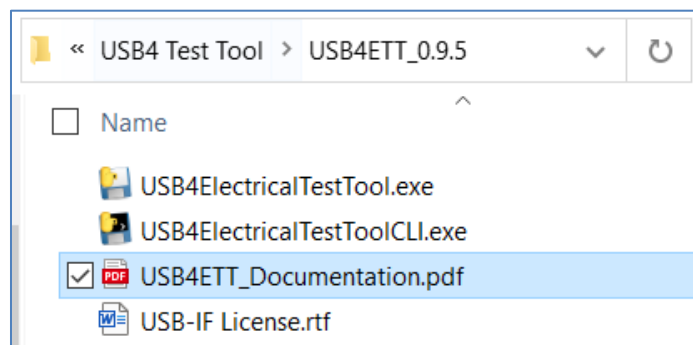

For USB4 Host Testing:

- The ETT can be loaded on the Control PC with the GRL-USB4RL-AN software. In this case, the Wilder-Tech μ Controller is required. The DUT is controlled using an Apple 0.8m USB Type-C® cable from the Wilder-Tech μ Controller to the Wilder-Tech USB4 Test Fixture.

For USB4 Device Testing:

- Upstream Facing Port (UFP):** The ETT can be loaded on the Control PC with the GRL-USB4RL-AN software. In this case, the Wilder-Tech μ Controller is required. The DUT is controlled using an Apple 0.8m USB Type-C cable from the Wilder-Tech μ Controller to the Wilder-Tech USB4 Test Fixture.
- Downstream Facing Port (DFP):** Connect the DUT's UFP to any USB4 host via the USB4 based USB-C® cable. The ETT tools can be loaded on the Control PC with the GRL-USB4RL-AN software. In this case, the Wilder-Tech μ Controller is required. The DUT is controlled using an Apple 0.8m USB Type-C cable from the Wilder-Tech μ Controller to the Wilder-Tech USB4 Test Fixture.

**Disclaimer: USB Type-C® and USB-C® are registered trademarks of USB Implementers Forum.*

3.1.3 Launch and Set Up Software

3.1.3.1 On the Control PC

1. Launch GRL Platform Solutions Host Application from Start Menu -> GRL -> GRL – Automated Test Solutions.
2. Select Application -> Framework Test Solution -> Anritsu USB4 Return Loss Test Application.
3. Type in the IP Address of the Anritsu VNA into the “Address” field and click the “lightning” button . The “lightning” button should turn green  if successfully connected to the equipment.

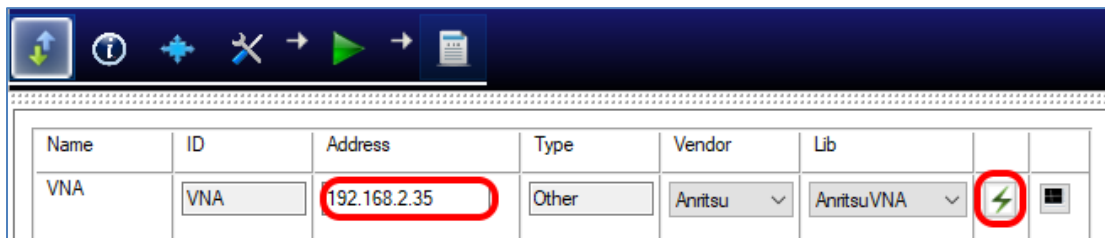


FIGURE 7. GRL-USB4RL-AN IP ADDRESSING ON VNA

3.1.3.2 Session Info

Select the  button in the main software menu to access the Session Info page. The information provided will be included in the report.

- The **DUT Info** and **Test Info** are input by the user.
- The **Software Info** is automatically populated.

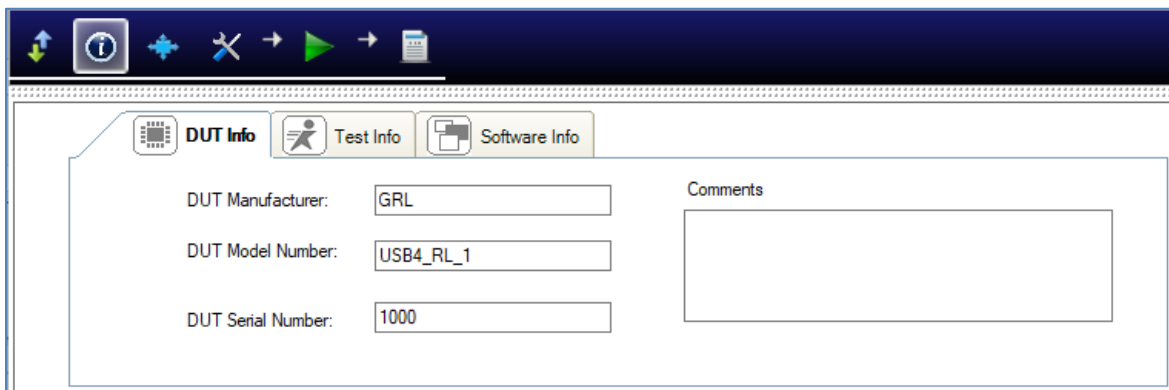


FIGURE 8. SESSION INFO PAGE

3.1.3.3 Test Conditions

Select the  button in the main software menu to access the Test Conditions page.

a) **Test Port tab:** Select the test ports on the device under test.

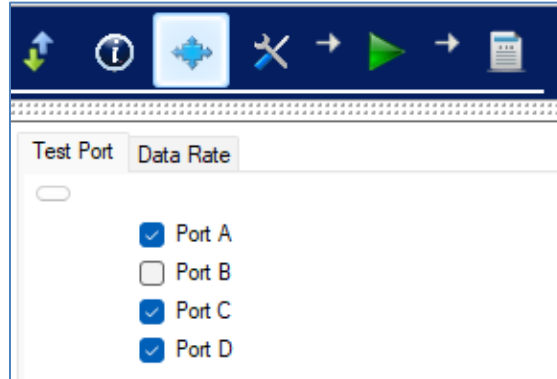


FIGURE 9. SELECT TEST PORT

b) **Data Rate tab:** Select the desired data rate.

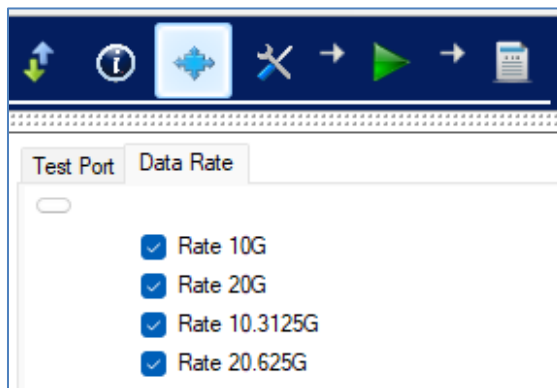


FIGURE 10. SELECT DATA RATE

4 Time and Frequency Domain Calibration Setups

Calibration is to be performed for RF effects such as delay, loss or mismatch of RF cables and SMA-SMP adapters using “SOLT” and “Reference Plane” calibration methods before running measurements. Calibration must be performed for both the time domain (Channel 1) and frequency domain (Channel 2).

Note: The test fixture is not used for calibration.

The figures below show the calibration setup diagrams for time and frequency domain, which require the Anritsu TOSLKF50A-20 VNA calibration kit and Rosenberger SMP jack adapters.

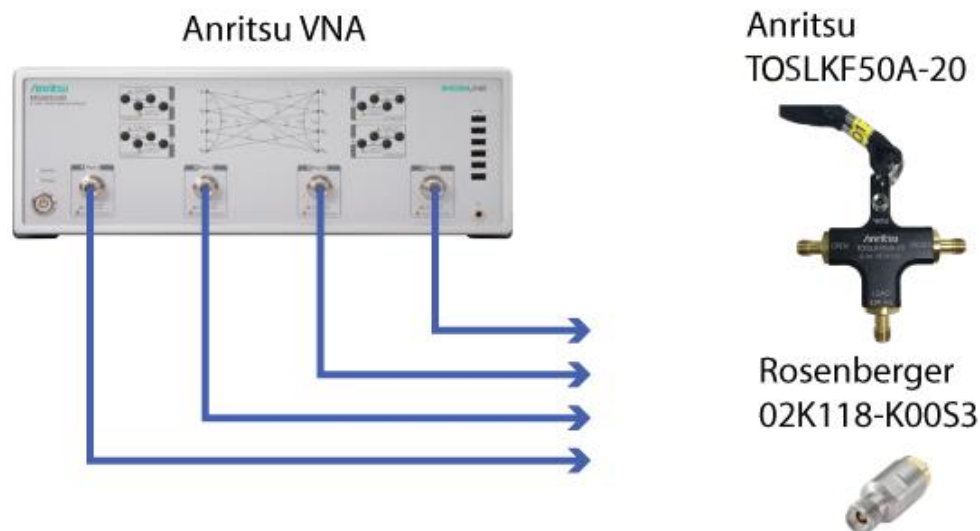


FIGURE 11. CALIBRATION SETUP FOR TIME DOMAIN CALIBRATION


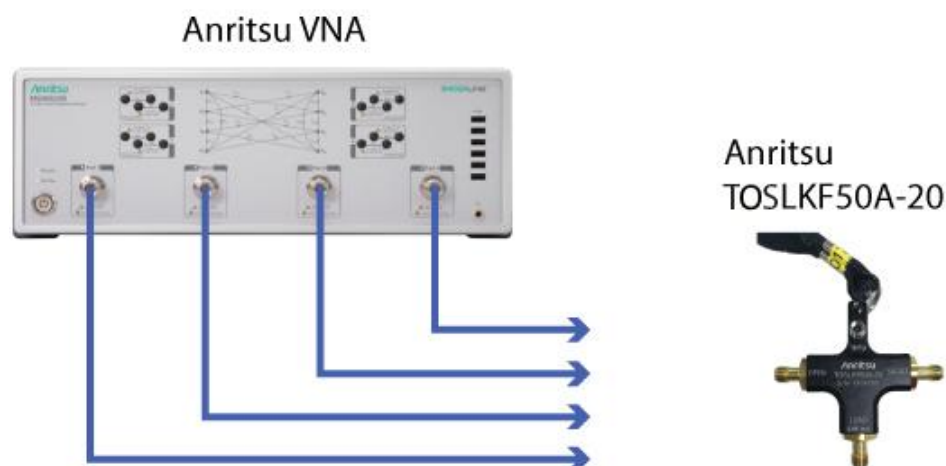


FIGURE 12. CALIBRATION SETUP FOR FREQUENCY DOMAIN CALIBRATION

Note: The Anritsu TOSLKF50A-20 VNA calibration kit is required for SOLT calibration, while the Rosenberger SMP jack adapters are required for Reference Plane calibration.

The GRL-USB4RL-AN software will guide user step by step on how to connect the equipment and perform the SOLT calibration and Reference Plane calibration.

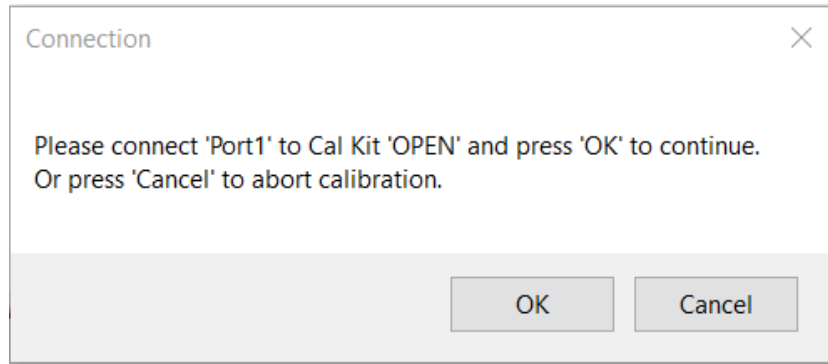

The following shows another pop-up example by the GRL-USB4RL-AN software to guide user to connect the SMP jack adapters to perform the Reference Plane calibration.

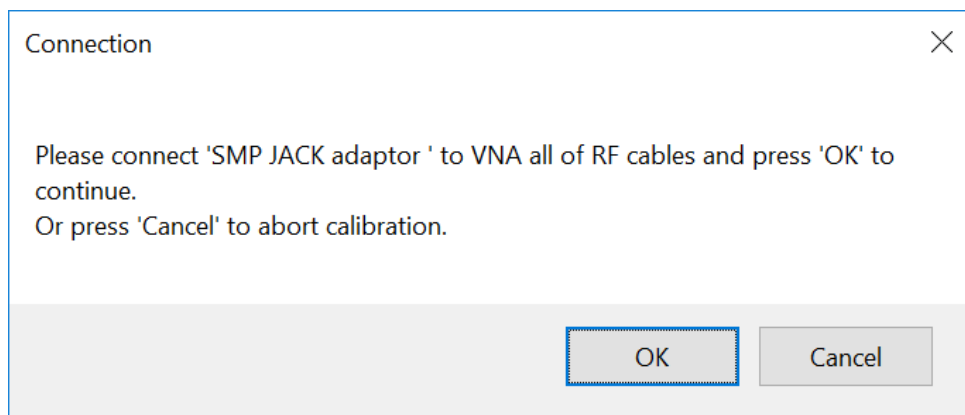


FIGURE 13. SOFTWARE CALIBRATION GUIDE EXAMPLE

5 Calibrating with GRL-USB4RL-AN Software

5.1 Select Calibration

The Select Tests page is the place where the calibration and tests that need to be performed are selected. Initially, when starting for the first time or changing anything in the setup, it is suggested to run Calibration first. If calibration is not completed, the tests will show an error message.


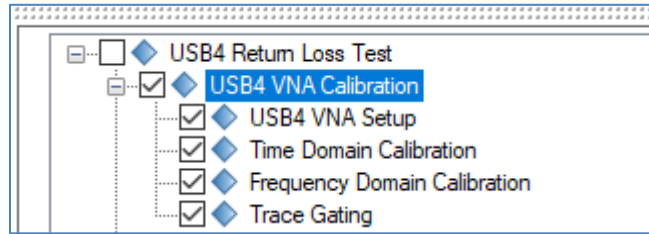


FIGURE 14. SELECT CALIBRATION TYPES

Note: Trace Gating is only applicable for the **SMP** fixture. In the Configurations  page, select the SMP fixture in the “Fixture Type” field as follows:

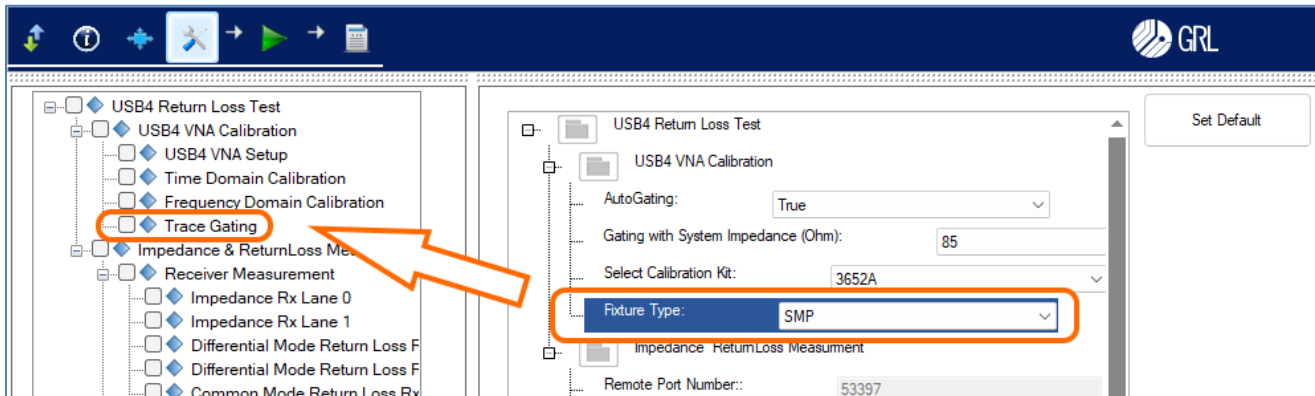

Refer to Section 5.2, Configure Calibration Parameters for more information.

Select the USB4 VNA Calibration group to set up the VNA test environment and perform time and frequency domain calibration and trace gating. The GRL-USB4RL-AN software will guide the user step by step while calibration is being run.

Note: All calibrations must be performed for both the time domain and frequency domain.

5.2 Configure Calibration Parameters

Select the  button in the main software menu to access the Configurations page. Set the parameters required for the calibration setup.

To return all parameters to their default values, select the 'Set Default' button.

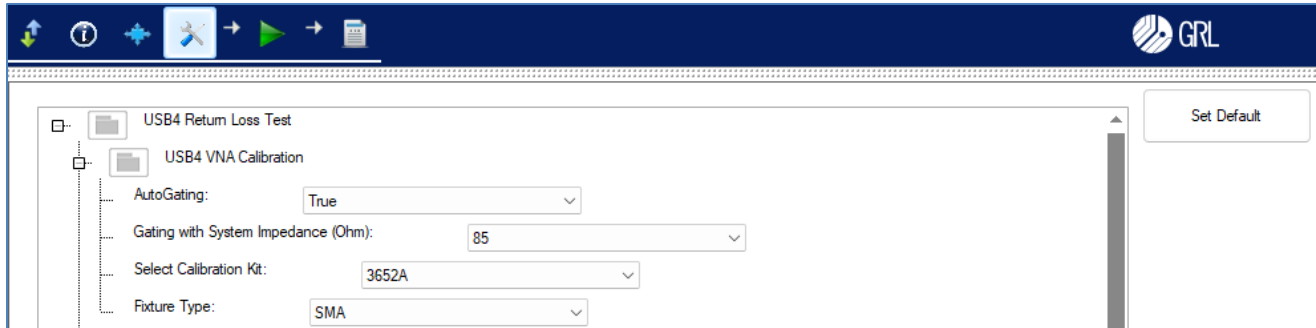
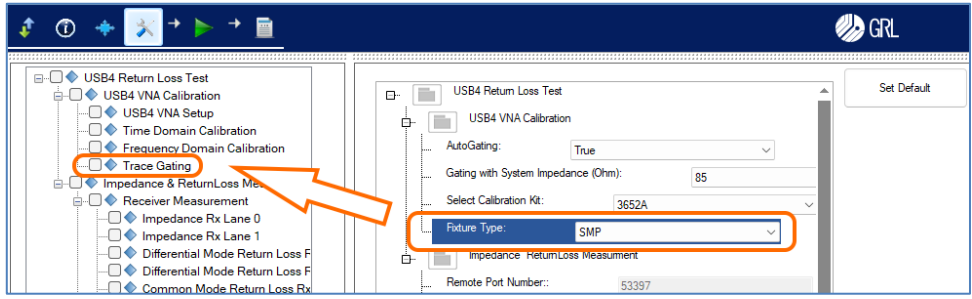


FIGURE 15. CALIBRATION CONFIGURATION PAGE

TABLE 4. CALIBRATION PARAMETERS

Parameter	Description
AutoGating	Select 'True' to enable auto gating method when performing trace gating.
Gating with System Impedance (Ohm)	Select to apply 85 or 100 ohms impedance for trace gating. For compliance testing, 85 ohms should be selected for both calibration and testing.
Select Calibration Kit	Select the calibration kit as supported by the GRL-USB4RL-AN software – Anritsu TOSLK50A-20 Calibration Kit or Anritsu 3652A K Connector Calibration Kit, to be used.
Fixture Type	Select the SMA or SMP jack adapter to be used with the calibration kit. To perform trace gating, SMP needs to be selected. This will cause the Trace Gating selection to appear in the calibration list as follows: 

5.3 Run Calibration

Select the  button in the main software menu to access the Run Tests page.

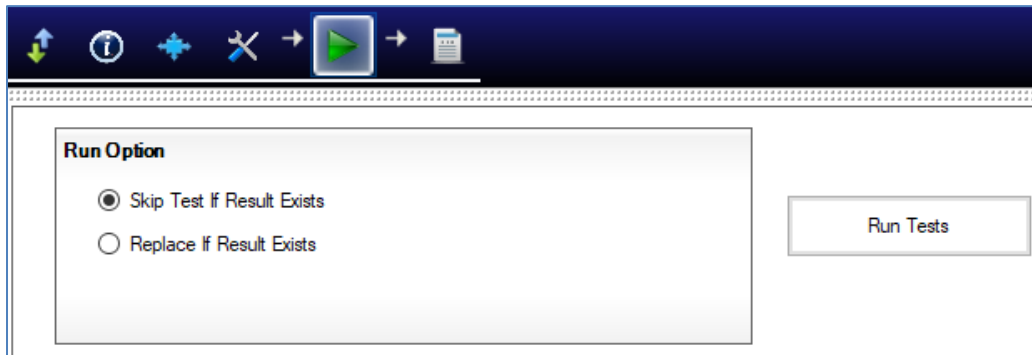


FIGURE 16. RUN TESTS PAGE

TABLE 5. RUN OPTIONS

Run Option	Description
Skip Test if Result Exists	If previous test or calibration results exist, then the software will <i>skip</i> the tests/calibration steps that have existing reports.
Replace if Result Exists	If previous test or calibration results exist, then the software will replace each step in the test/calibration with new results.

If you need to re-run only certain calibration/tests on certain conditions, please delete the calibration/tests from the Report page (see Section 9.2 for example) and Run with **Skip Test if Result Exists**. The GRL-USB4RL-AN software will keep track of the missing calibration/tests in the report and perform those tests only.

6 Configure Proper Setup in Configurations Menu

After calibration has completed, testing for DUT compliance can then be performed. The USB4 Return Loss VNA test setup consists of Impedance measurement (informative) and Return Loss measurement on receiver/transmitter lanes of the DUT. The USB4 ETT as listed in Section 2.2 is required to run the automation tests.

Refer to Section 3.1.2 for options on how to configure the test setup. The ETT can be loaded on the control PC. The Wilder-Tech μ Controller can be used to test any Host or Device Port. Take note for the device DUT, if the port under test is a Downstream Facing Port (DFP), a USB4 Host will be required to connect to the DUT's Upwards Facing Port (UFP). Follow the steps in the below section for setup depending on the configuration chosen.

Note that careful handling is needed when making coaxial connections on to the test fixture. Refer to the Wilder-Tech user documentation for detailed precautions (see Section 2.1).

6.1 Host DUT Setup

If testing a Host, and the ETT have been loaded on the Control PC, and the μ Controller has been connected to the Control PC via a USB cable, follow the below procedure:

1. Connect the equipment as follows:


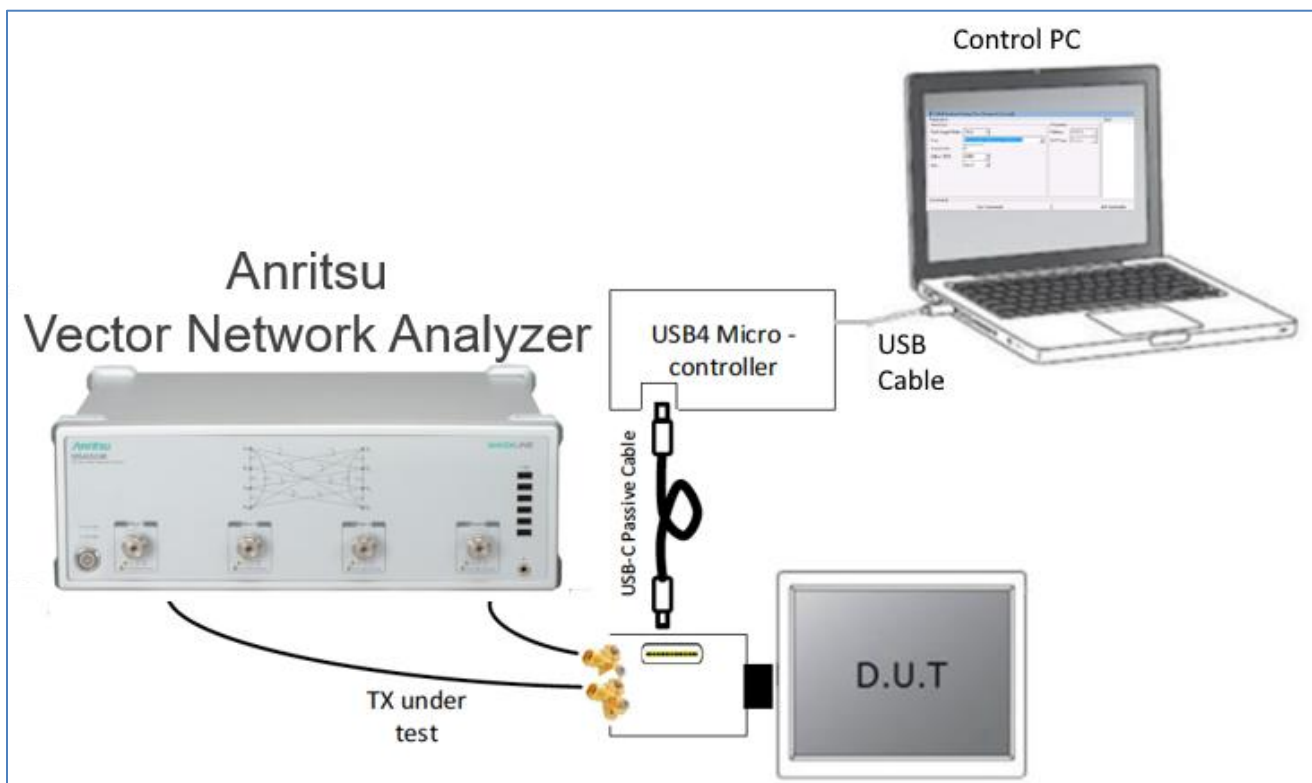


FIGURE 17. TEST SETUP FOR HOST DUT

2. On the main GRL-USB4RL-AN software menu, select the  button to access the Configurations page.

- Select “Host” in the “DUT Type” field.
- Select “uController” in the “USB4 Electrical Scripts Controller” field.
- Select “ETT” in the “Test Script Version” field.
- Specify the directory of the ETT on the Host DUT in the “uController Working Directory” field.

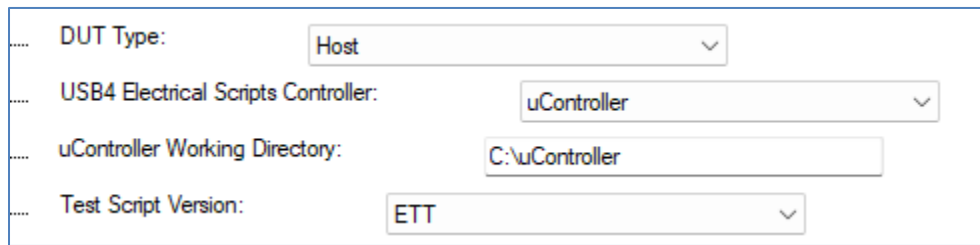

The screenshot shows the configuration window with the following settings:

- DUT Type:** Host
- USB4 Electrical Scripts Controller:** uController
- uController Working Directory:** C:\uController
- Test Script Version:** ETT


FIGURE 18. CONFIGURE HOST DUT EXAMPLE IN GRL-USB4RL-AN SOFTWARE

6.2 Device DUT Setup for UFP

If testing a Device’s UFP, connect the equipment similar to the Host DUT setup in Section 6.1. Then, follow the below procedure:

On the main GRL-USB4RL-AN software menu, select the  button to access the Configurations page.

- Select “Device” in the “DUT Type” field.
- Select “uController” in the “USB4 Electrical Scripts Controller” field.
- Select “ETT” in the “Test Script Version” field.
- Specify the directory of the ETT on the USB4 remote host in the “uController Working Directory” field.

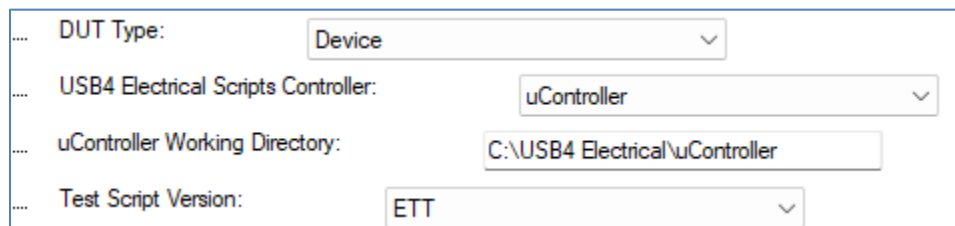

The screenshot shows the configuration window with the following settings:

- DUT Type:** Device
- USB4 Electrical Scripts Controller:** uController
- uController Working Directory:** C:\USB4 Electrical\uController
- Test Script Version:** ETT

FIGURE 19. CONFIGURE DEVICE DUT (UFP) EXAMPLE IN GRL-USB4RL-AN SOFTWARE

6.3 Device DUT Setup for DFP

If testing a Device’s DFP, connect the equipment similar to the Host DUT setup in Section 6.1. Take note that the DUT’s UFP should be connected to a USB4 host port.

Follow the same procedure as for the Device’s UFP setup in Section 6.2 above.

7 Perform Trace Gating

Trace gating can be performed to remove SMP connector effects between the SMP jack adapter and the test fixture.

Note: Prior to running trace gating, make sure that the above relevant test setup (Section 6.1 to 6.3) has been completed.

1. On the Select Tests page, select “Trace Gating”.


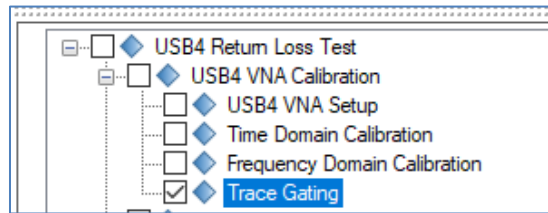


FIGURE 20. SELECT TRACE GATING

Note: Trace Gating is only applicable for the **SMP** fixture. In the Configurations  page, select the SMP fixture in the “Fixture Type” field as follows:

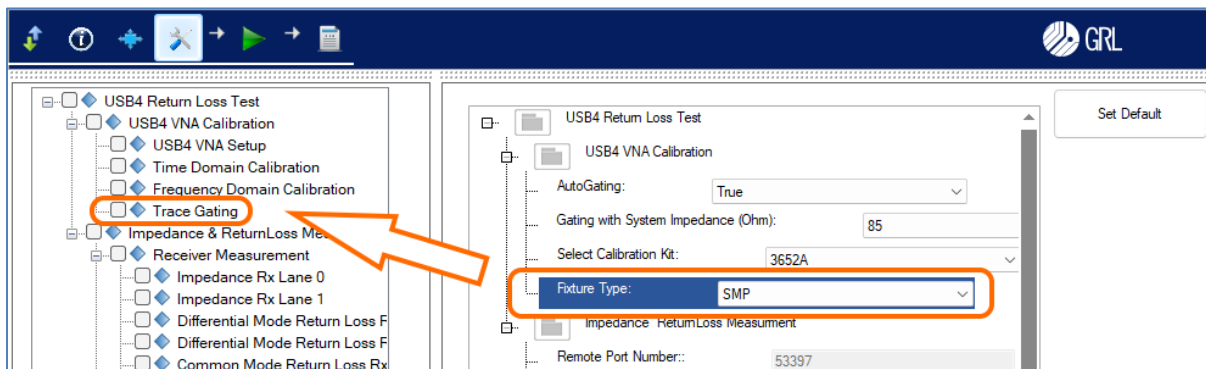

Refer to Section 5.2, Configure Calibration Parameters for more information.

2. Click “Run Tests” under  to start running trace gating.

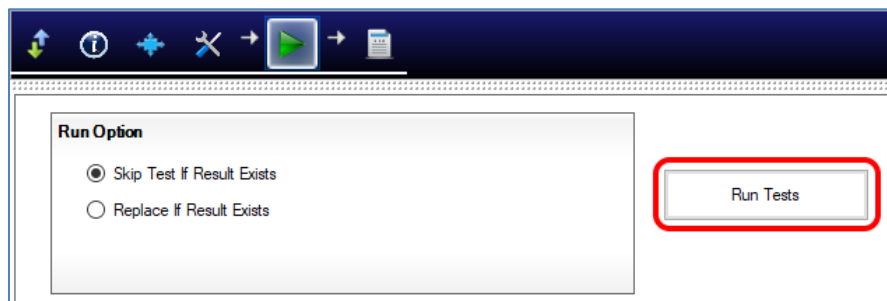


FIGURE 21. RUN TRACE GATING

3. Follow the software instructions step by step to complete the process.

8 DUT Compliance Testing with GRL-USB4RL-AN Software

8.1 Select Tests

On the Select Tests page, un-check all Calibration Selections as they have been performed and completed in the previous section. Then select the tests required to be run.

Note: GRL Platform Solutions recommends running Rx and Tx Tests Separately in this version of GRL-USB4RL-AN. Otherwise for each data rate a prompt will come up to change from Rx to Tx on the Fixture. If Rx and Tx are tested separately, then all Rx will be tested and then all Tx will be tested with only one change needed to the fixture.

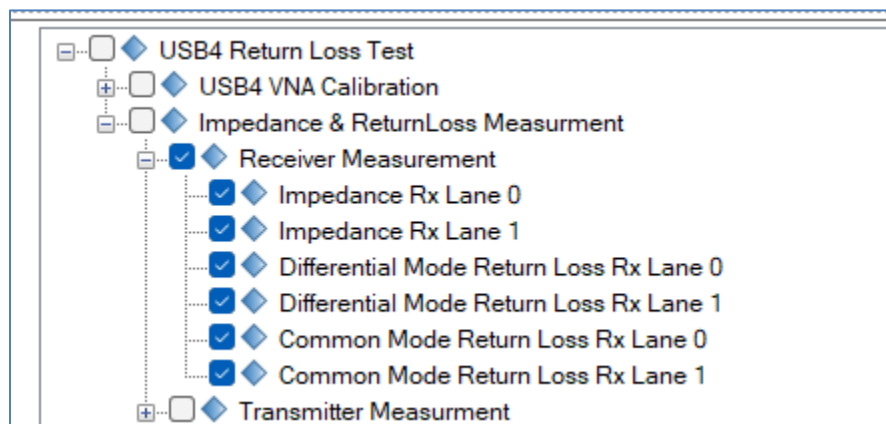


FIGURE 22. SELECT RX MEASUREMENT TESTS

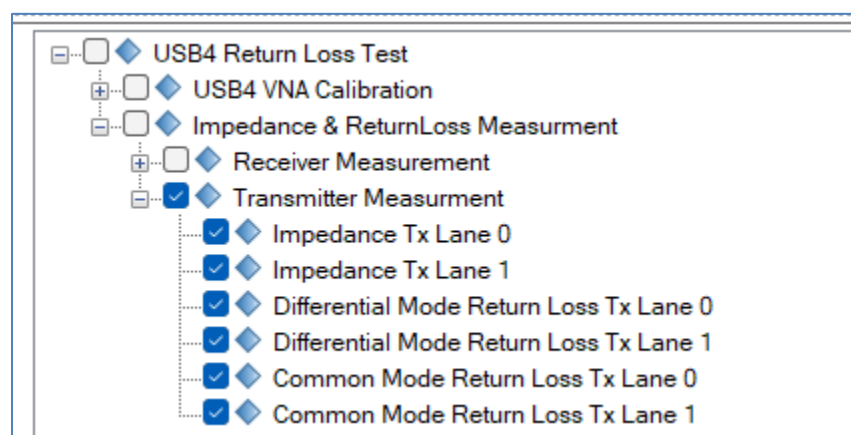


FIGURE 23. SELECT TX MEASUREMENT TESTS

8.2 Configure Test Parameters

Select the  button in the main software menu to access the Configurations page. Set the parameters required for the test setup.

To return all parameters to their default values, select the 'Set Default' button.

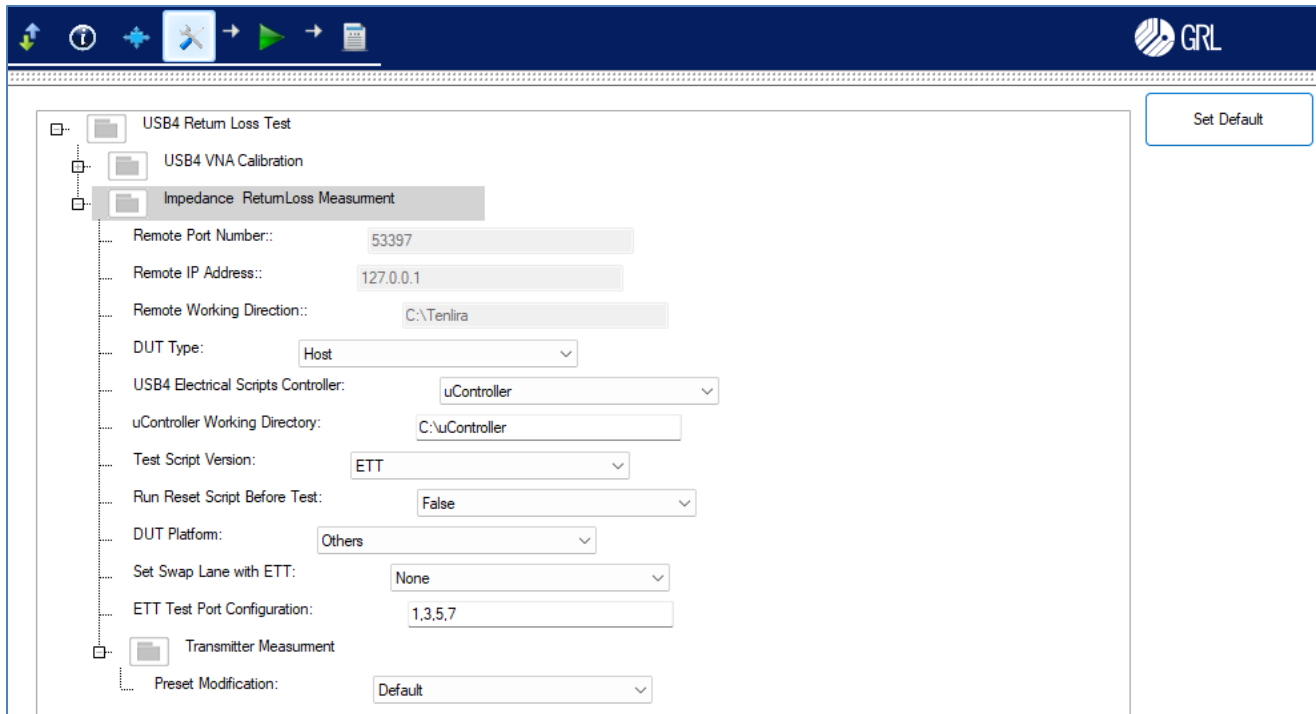


FIGURE 24. TEST CONFIGURATION PAGE

TABLE 6. TEST PARAMETERS

Parameter	Description
DUT Type	Select this first. Select whether DUT is Host or Device or Tethered Device (if DUT has tethering capability).
USB4 Electrical Scripts Controller	Select this second. Select whether port will be controlled by Remote Thunderbolt 3 Host or uController or JTAG (if DUT supports JTAG technology) or manually.
Remote Port Number	If DUT Controlled By: Remote TBT3 Host and DUT is TBT3 , specify the remote server's port number of the controller host of the test script.
Remote IP Address	If DUT Controlled By: Remote TBT3 Host and DUT is TBT3 , specify the remote server's IP address of the controller host of the test script.
Remote Working Directory	If DUT Controlled By: Remote TBT3 Host and DUT is TBT3 , set the working directory to the path where the test script is installed in the remote controller host.
uController Working	If DUT Controlled By: uController , set the working directory to

Directory	the path where the μ Controller test script or ETT is installed on the control PC.
Test Script Version	Select ETT to run ETT or 0.8.6 and above to run Tenlira script.
Run Reset Script Before Test	Select True to enable the GRL-USB4RL-AN software to reset the μ Controller before running the test script or ETT command each time.
DUT Platform	Select the platform/processor as supported by the DUT for running test scripts.
Set Swap Lane with ETT	If ETT is selected from the “Test Script Version” field, select the Swap Lane(s) in the Router and/or Retimer side (“None” is selected by default).
ETT Test Port Configuration	If ETT is selected from the “Test Script Version” field and if the Device DUT is being used, specify the ETT API argument “-Dp”(DUT Test Port), {PortA,PortB,PortC,PortD}
Preset Modification	Select the default or any of the 16 transmitter equalization presets when changes to the preset is required during transmitter measurements.

8.3 Performing Impedance and Return Loss Measurement

The following example describes how to measure impedance and return loss. Impedance is measured at the time domain while return loss is measured at the frequency domain. Measurement should be performed on both the transmitter and receiver lanes.

Note: The impedance measurement is carried out for information purpose only, meaning it has no test limit specification.

Note: Prior to running measurements, make sure that the relevant test setup described in Section 6 has been completed.

1. Select the  button in the main GRL-USB4RL-AN software menu to access the Run Tests page and click “Run Tests”. Select whether to Skip existing results or Replace if results exist.


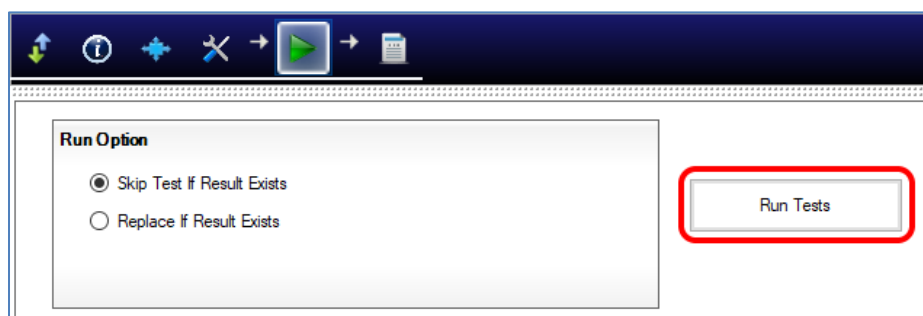


FIGURE 25. RUN TESTS PAGE

2. Follow the software instructions step by step to set up the connection and run the selected tests.

3. Once tests have completed, the test results will be saved automatically and

populated on the Report page (select the  button on the main GRL-USB4RL-AN software menu). Click “Generate report” to view the details of each result.

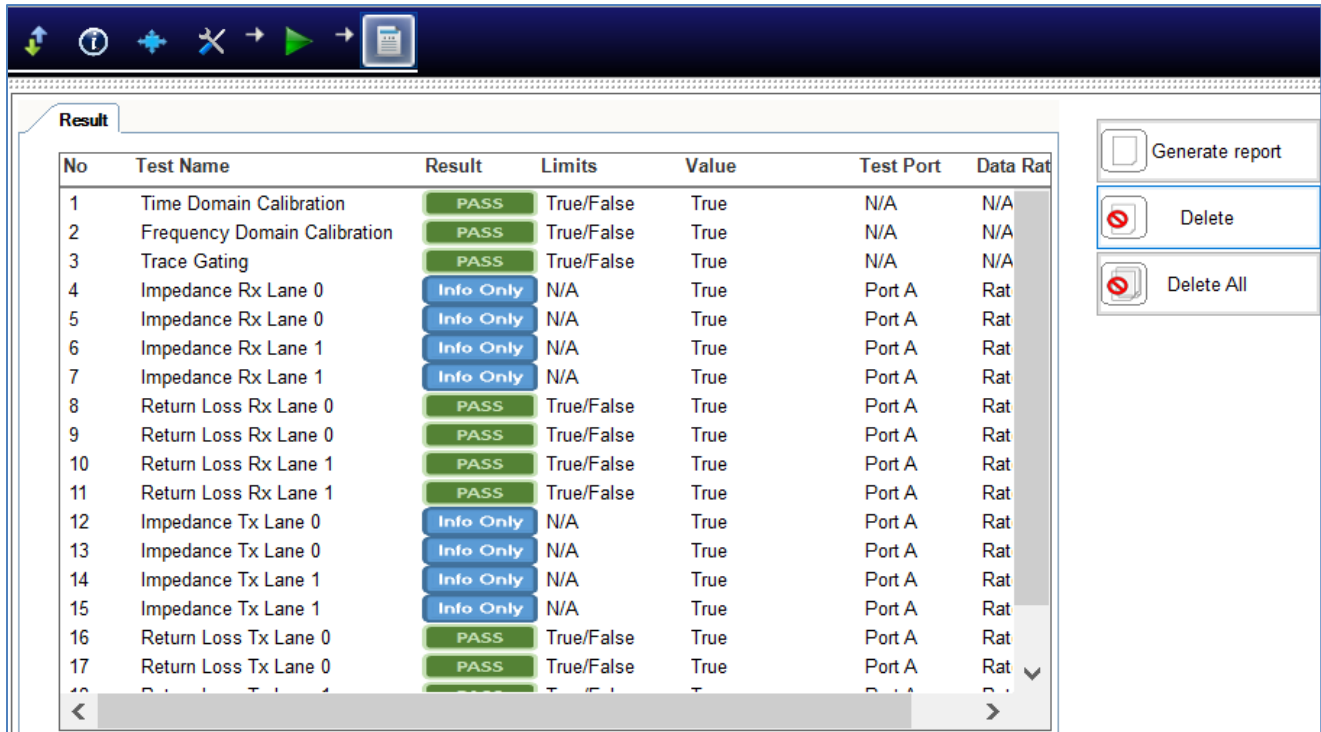

No	Test Name	Result	Limits	Value	Test Port	Data Rate
1	Time Domain Calibration	PASS	True/False	True	N/A	N/A
2	Frequency Domain Calibration	PASS	True/False	True	N/A	N/A
3	Trace Gating	PASS	True/False	True	N/A	N/A
4	Impedance Rx Lane 0	Info Only	N/A	True	Port A	Rat
5	Impedance Rx Lane 0	Info Only	N/A	True	Port A	Rat
6	Impedance Rx Lane 1	Info Only	N/A	True	Port A	Rat
7	Impedance Rx Lane 1	Info Only	N/A	True	Port A	Rat
8	Return Loss Rx Lane 0	PASS	True/False	True	Port A	Rat
9	Return Loss Rx Lane 0	PASS	True/False	True	Port A	Rat
10	Return Loss Rx Lane 1	PASS	True/False	True	Port A	Rat
11	Return Loss Rx Lane 1	PASS	True/False	True	Port A	Rat
12	Impedance Tx Lane 0	Info Only	N/A	True	Port A	Rat
13	Impedance Tx Lane 0	Info Only	N/A	True	Port A	Rat
14	Impedance Tx Lane 1	Info Only	N/A	True	Port A	Rat
15	Impedance Tx Lane 1	Info Only	N/A	True	Port A	Rat
16	Return Loss Tx Lane 0	PASS	True/False	True	Port A	Rat
17	Return Loss Tx Lane 0	PASS	True/False	True	Port A	Rat
18	Return Loss Tx Lane 1	PASS	True/False	True	Port A	Rat

FIGURE 26. VIEW TEST RESULTS EXAMPLE

9 Test Results and Reports with GRL-USB4RL-AN Software

The **Report**  page displays all the results from all test and calibration runs. If some of the results are not desired, they can be individually deleted by clicking the “Delete” button. Also for a PDF report, select the “Generate report” button.

9.1 Generate Test Report

The Report page shows all the results of tests and calibration. Select **Generate report** for the detailed report.

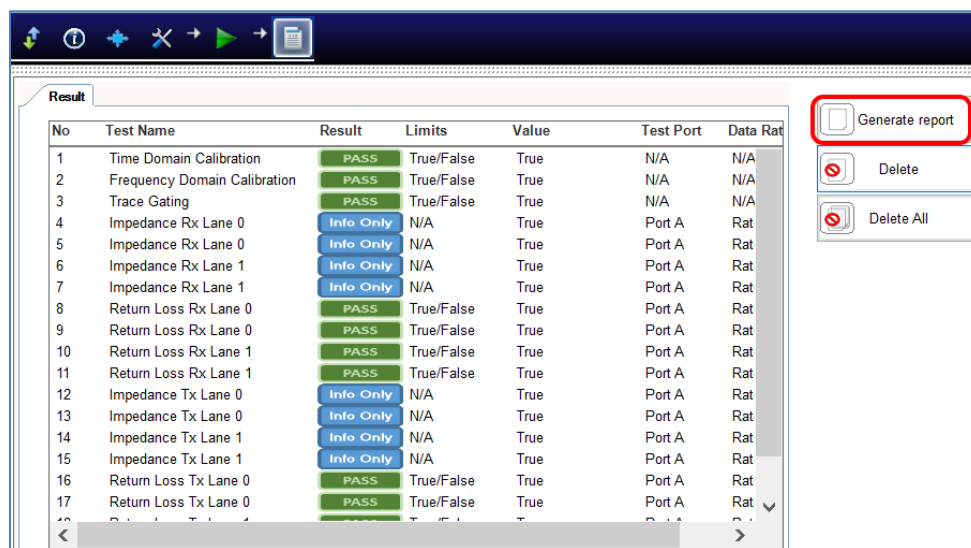


FIGURE 27. GENERATE REPORT PAGE

9.1.1 DUT Information

This portion is populated from the information in the DUT tab on the **Session Info** page.

Anritsu USB4 Return Loss Test Application Report	
DUT Information	
DUT Manufacturer	: GRL
DUT Model Number	: USB4_RL_1
DUT Serial Number	: 1000
DUT Comments	:
Test Information	
Test Lab	: Granite River Labs
Test Operator	: David
Test Date	: 1 Oct 2020
Software Version	
Software Revision	: 0.0.0.1

FIGURE 28. DUT INFORMATION

9.1.2 Summary Table

This portion is populated from the tests and calibration performed and their results. This gives a summarized view of all the results and test conditions.

Anritsu USB4 Return Loss Test Application Report						
No	TestName	Limits	Value	Results	Test Port	Data Rate
1	USB4 VNA Setup	N/A	N/A	Pass		
2	Time Domain Calibration	N/A	N/A	Pass		
3	Frequency Domain Calibration	N/A	N/A	Pass		
4	Trace Gating	N/A	N/A	Pass		
5	Impedance Rx Lane 0	N/A	N/A	InfoOnly	PortA	Rate10G
6	Impedance Rx Lane 0	N/A	N/A	InfoOnly	PortA	Rate20p6G
7	Impedance Rx Lane 1	N/A	N/A	InfoOnly	PortA	Rate10G
8	Impedance Rx Lane 1	N/A	N/A	InfoOnly	PortA	Rate20p6G
9	Differential Mode Return Loss Rx Lane 0	N/A	N/A	Pass	PortA	Rate10G
10	Differential Mode Return Loss Rx Lane 0	N/A	N/A	Pass	PortA	Rate20p6G
11	Differential Mode Return Loss Rx Lane 1	N/A	N/A	Pass	PortA	Rate10G
12	Differential Mode Return Loss Rx Lane 1	N/A	N/A	Pass	PortA	Rate20p6G
13	Impedance Tx Lane 0	N/A	N/A	InfoOnly	PortA	Rate10G
14	Impedance Tx Lane 0	N/A	N/A	InfoOnly	PortA	Rate20G
15	Impedance Tx Lane 1	N/A	N/A	InfoOnly	PortA	Rate10G
16	Differential Mode Return Loss Tx Lane 0	N/A	N/A	Pass	PortA	Rate10G
17	Differential Mode Return Loss Tx Lane 1	N/A	N/A	Pass	PortA	Rate10G

FIGURE 29. SUMMARY TABLE

9.1.3 Test Result Details

This portion is populated from each of the test and calibration results. Here the results are explained in depth with supporting data points and screenshots.



FIGURE 30. TEST RESULT DETAILS EXAMPLE

9.2 Delete Reports

If some of the results are not desired, they can be individually deleted by selecting the “Delete” button.

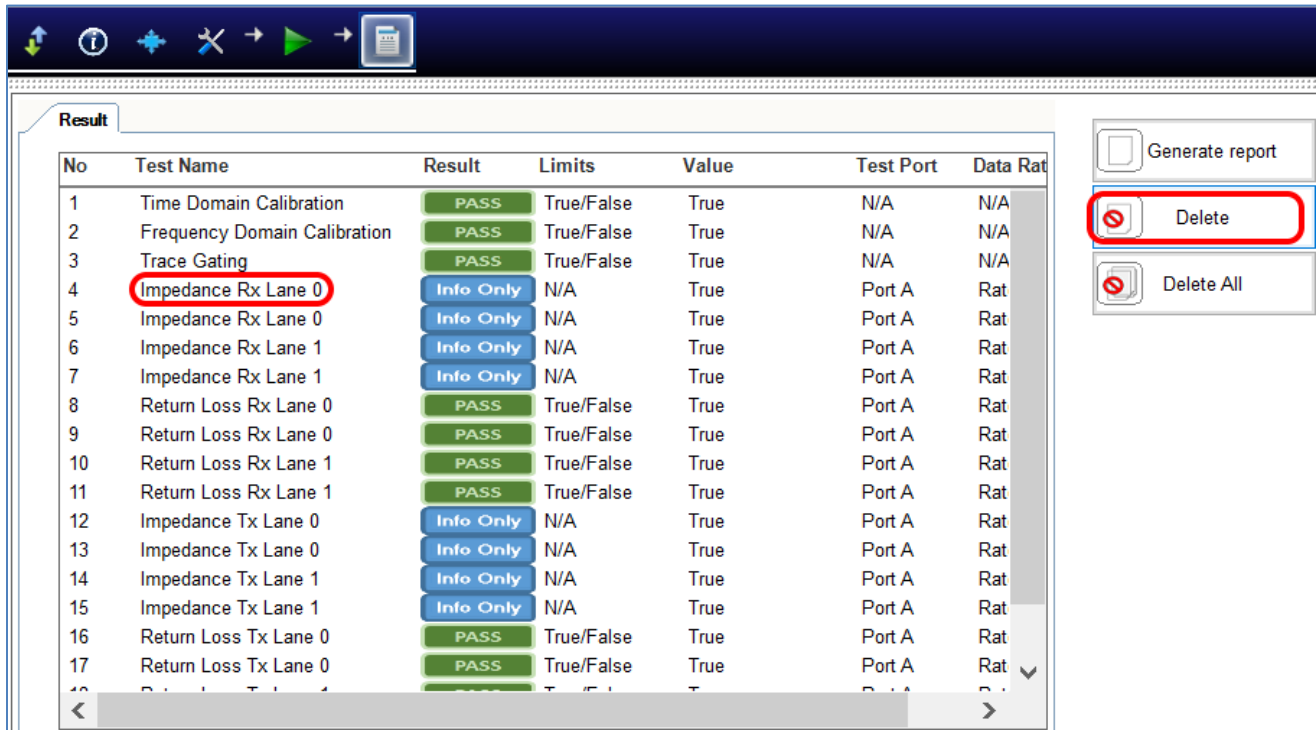


FIGURE 31. DELETE INDIVIDUAL CALIBRATION/TEST RESULTS EXAMPLE

To remove all results, select the “Delete All” button.

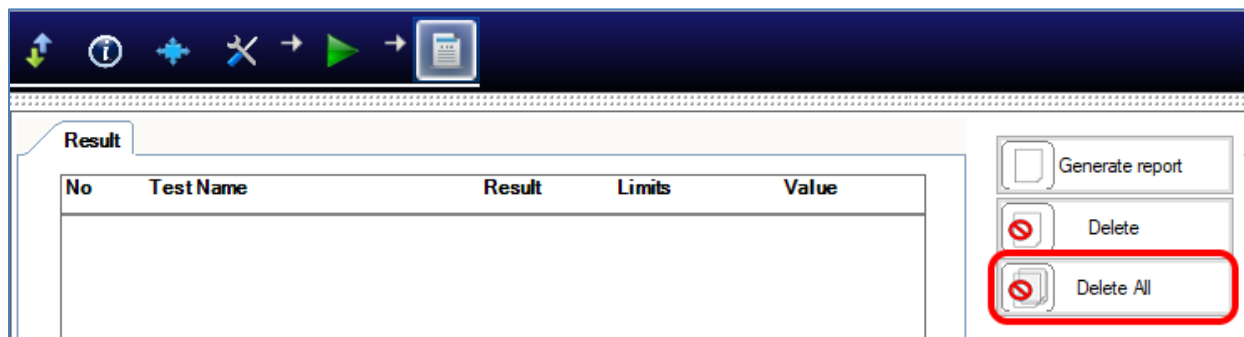


FIGURE 32. DELETE ALL RESULTS

10 Troubleshooting GRL-USB4RL-AN Errors

If an error is thrown by the GRL-USB4RL-AN software, it may be due to one of the following common issues:

1. The VNA's firmware needs to be updated – Confirm that the VNA's firmware is V2018.2.1 or above.
2. USB4 ETT is not properly installed – To troubleshoot this, follow the ETT PDF User Guide and confirm that **USB4ElectricalTestTool.exe** can be run manually from the ETT folder. If ETT is not properly installed, a software error may occur.
3. After checking the above and error persists, contact support@grlps.com for further support.

END_OF_DOCUMENT